(51) International Patent Classification 5 :		(11) International Publication Number: **WO 92/00699**
A61B 5/00	**A1**	(43) International Publication Date: 23 January 1992 (23.01.92)

(71) Applicant *(for all designated States except US)*: IMPERIAL COLLEGE OF SCIENCE TECHNOLOGY AND MEDICINE [GB/GB]; Prince Consort Road, London SW7 2BZ (GB).

(72) Inventors; and
(75) Inventors/Applicants *(for US only)* : GENEVIER, Eric, Serge, Gilles [FR/GB]; 81 Clifford Gardens, London NW10 5JG (GB). STEER, Philip, James [GB/GB]; 97 Blenheim Gardens, Kingston upon Thames, Surrey KT2 7BJ (GB). DANIELIAN, Peter, James [GB/GB]; 28 Horsford Road, London SW2 5BM (GB). RANDALL, Nigel, John [GB/GB]; 30 Carlisle Road, London NW6 6TS (GB). SMITH, Robin, Wyncliffe [GB/GB]; Optics Section, Blackett Laboratory, Imperial College of Science Technology and Medicine, Prince Consort Road, London SW7 2BZ (GB).

(54) Title: MECONIUM MONITORING SYSTEM
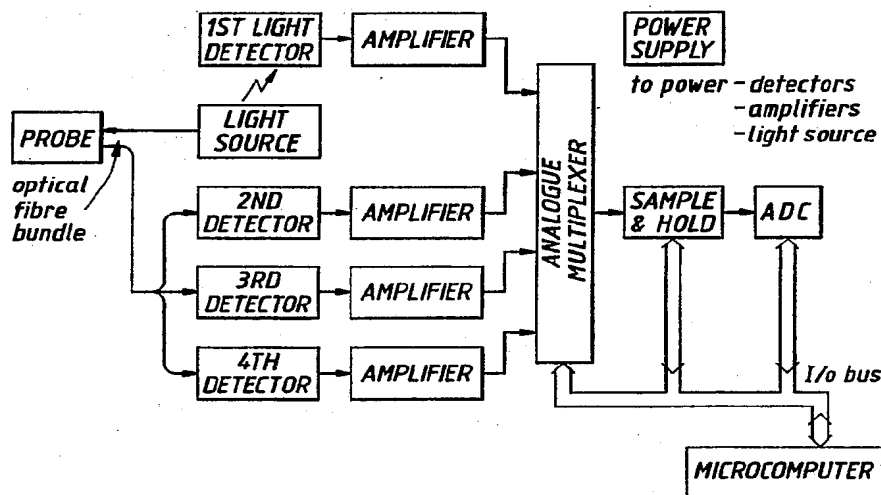
(57) Abstract

A system is disclosed for *in vivo* monitoring of the presence and concentration of meconium and/or blood in amniotic fluid. One aspect of the invention provides a non-invasive system for monitoring the content of amniotic fluid during labour which comprises an optical cell (31) supported in a probe (32) capable of insertion into the uterus during labour, said cell being connected optically to a source of light (having a suitable spectral bandwidth) and to photodetecting means for detecting the spectral response of the amniotic fluid to illumination with said source and processing means for determining the presence of meconium and/or blood in the amniotic fluid by analysis of the spectral response. The invention includes an intrauterine probe (32) which comprises a flexible elongated body and an optical cell (31) housed therein, the cell being optically connected by fibre optic cable (33) to the distal end and the cell being located in the housing so that in use amniotic fluid is able to pass through the cell.

+ See back of page

+ DESIGNATIONS OF "SU"

It is under examination in which parts of the former Soviet Union the designation of the Soviet Union has effect.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	ES	Spain	MG	Madagascar
AU	Australia	FI	Finland	ML	Mali
BB	Barbados	FR	France	MN	Mongolia
BE	Belgium	GA	Gabon	MR	Mauritania
BF	Burkina Faso	GB	United Kingdom	MW	Malawi
BG	Bulgaria	GN	Guinea	NL	Netherlands
BJ	Benin	GR	Greece	NO	Norway
BR	Brazil	HU	Hungary	PL	Poland
CA	Canada	IT	Italy	RO	Romania
CF	Central African Republic	JP	Japan	SD	Sudan
CG	Congo	KP	Democratic People's Republic	SE	Sweden
CH	Switzerland		of Korea	SN	Senegal
CI	Côte d'Ivoire	KR	Republic of Korea	SU	Soviet Union
CM	Cameroon	LI	Liechtenstein	TD	Chad
CS	Czechoslovakia	LK	Sri Lanka	TG	Togo
DE	Germany	LU	Luxembourg	US	United States of America
DK	Denmark	MC	Monaco		

MECONIUM MONITORING SYSTEM

This application relates to a system and method for monitoring the quality of amniotic fluid during labour.

In recent years, it has become accepted that there is a need for more information concerning the condition within the uterus just prior to and during labour in order to predict and avoid birth complications. U.K. Patent Application No. 87 23605 (Publication No. 2195897) describes an intrauterine probe which enables certain conditions, especially the fetal heart rate and the intrauterine pressure to be continuously monitored during labour. Any monitoring system should desirably be non-invasive to the fetus and be capable of a continuous collection of data concerning the condition of interest.

During intrauterine life, the human fetus collects within its bowel a collection of debris known as meconium. Passage of meconium in utero occurs in about 10% of babies overall, probably as part of a sympathetic 'fright, flight or fight' reaction. Because regular uterine contractions interfere with maternal blood flow within the placenta, the mean oxygen tension in fetal blood during labour drops from about 5 to 3kPa. This is thought to be the major stimulus causing the fetus to pass meconium in utero; it occurs with increasing frequency as gestation advances, reaching almost one third of all fetuses by 42 weeks gestation.

In 90% of fetuses who pass meconium into the amniotic fluid there are no harmful effects. However, in about 10% of cases the fetus gasps, inhaling the sticky, particulate meconium into the upper respiratory tract. Once the baby is born, this particulate matter produces partial airways obstruction, leading to inability to inflate alveoli in some areas, and hyperinflation in others. This disease is known as meconium aspiration syndrome (MAS).

Attempts have been made to prevent MAS by careful suctioning of the baby's pharynx immediately after the head is delivered; unfortunately such measures are largely ineffective.

It appears that there is, as yet, no known effective prevention of this crippling and disabling condition. The main factor preventing progress is that the appearance of meconium into the amniotic fluid often remains undetected because the tight fit of the head in the pelvis does not allow amniotic fluid to drain out and become visible to the attending obstetrician.

There is therefore a need for a method of reliably monitoring the onset of meconium passage into the amniotic fluid and particularly one which can be carried out non-invasively to the fetus and continuously throughout labour.

According to one aspect of the present invention,

there is provided a non-invasive system for monitoring the
content of amniotic fluid during labour which comprises an
optical cell supported in a probe capable of insertion
into the uterus during labour, said cell being connected
optically to a source of light (having a suitable spectral
bandwidth) and to photodetecting means for detecting the
spectral response of the amniotic fluid to illumination
with said source and processing means for determining the
presence of meconium and/or blood in the amniotic fluid by
analysis of the spectral response.

According to a second aspect of the present invention
there is provided an intrauterine probe which comprises a
flexible elongated body and an optical cell housed
therein, the cell being optically connected by fibre optic
cables to the distal end and the cell being located in the
housing in such a way that in use amniotic fluid is able
to pass through the cell.

Further features and advantages of the present
invention will become apparent from the following detailed
description and accompanying drawings in which:-

Figure 1 is an absorption spectrum of three samples
A, B & C of different amniotic fluids.

Figure 2 is an absorption spectrum of a blood-stained
sample of amniotic fluid with expected base line.

Figure 3 is a perspective diagrammatic view of an
intrauterine probe in accordance with the invention.

Figure 4 is an exploded view of an optical cell on an enlarged scale.

Figure 5 is a block diagram illustrating the signal processing equipment.

Two difficulties in making direct observations of the absorption spectrum of amniotic fluid are first to differentiate the spectra for meconium and blood, and secondly, to take into account the differing overall opacities between different samples of amniotic fluid. Typical spectra are shown in Figure 1, where A is the spectrum of a sample clear of meconium and blood, whereas B is the spectrum of a meconium stained sample showing a strong absorption peak in the range of 405 to 415nm, and C that of a blood stained sample. It can be seen that spectrum C has a major peak in the range of 405 to 415nm and two minor peaks in the range 535 to 545nm and 570 to 580nm.

The effect of blood on the absorption spectrum is important as it affects the whole spectrum in the range 405 to 415nm, where it adds a wide band peak in the same way as meconium does, the main difference between the two spectra being the two peaks seen at 540 and 575nm, and the fact that meconium absorbs poorly above about 650nm.

In order to account for the different opacities and distinguish between clear, meconium or blood-stained

amniotic fluid, the system and method of the present
invention involves a comparison of the spectral response
at different wavelengths.   One way in which this can be
done is to measure the absorption spectrum of the amniotic
fluid in the areas corresponding to the peaks produced by
meconium and blood and at a third wavelength which is
distant from the peaks characteristic of meconium and
blood.   In this way a base line value can be subtracted
from the peak absorption values of the fluid under test.
This procedure is illustrated graphically in Figure 2
which is a spectrum of a blood-stained sample of amniotic
fluid containing meconium.   It will be seen from Figure 2
that the point at 500nm can be taken as the base line.
From these three absorptances we can derive the following
variables:-

$$\delta(405) = K1 \cdot [A(405) - A(500)]$$

$$\delta(575) = K2 \cdot [A(500) - A(575)]$$

where :   A(405) = absorptance at 405nm

           A(500) = absorptance at 500nm

           A(575) = absorptance at 575nm

   These variables are referred to hereinafter as the
compensated absorptances.   K1 and K2 are arbitrary
constants to bring both values in the range 0 to 1.

   For a sample clear of meconium and blood, $\delta(405)$ and
$\delta(575)$ are both positive.   As the level of meconium is
increased, both $\delta(405)$ and $\delta(575)$ should increase but in

the case where blood is also present, $S(575)$ does not increase significantly and often decreases to become negative, this is because the addition to the spectrum of a peak at 575nm reduces the difference $A(500)-A(575)$.

Therefore, should blood appear in the amniotic fluid when meconium is already present, blood would immediately be detected, which is important as the appearance of blood in the amniotic fluid is a life-threatening condition requiring immediate attention.

While absorptance measurements can be used to discriminate amniotic fluid containing meconium or blood and clear fluid, a perfectly normal amniotic fluid may be extremely turbid because of the presence of vernix (a waxy substance which covers the fetus). In such circumstances, the vernix contamination makes it difficult to obtain meaningful absorptance measurements, except possibly in very thin films or after removal of a sample and centrifugation to clear the sample. The latter procedure is not usually possible where continuous monitoring is required.

A preferred procedure for analysing the spectral response of the amniotic fluid to illumination involves measurement of light back scattered (i.e. reflecte from a sample of the fluid. An amniotic fluid which is contaminated with vernix has a milky appearance and reflects light strongly over a wide waveband. As meconium

increases in the amniotic fluid, it is also responsible for scattering light. Further, increased turbidity of the fluid will result in a reflected signal of increased strength.

It is, however, possible to distinguish increases in reflectance due to the presence of meconium, as opposed to vernix or other contaminants, by exploiting the optical absorptance characteristics of meconium as mentioned above. Because meconium absorbs light in the range of about 402 to 420nm, measurement of reflected values in this waveband compared with reflectance values at a wavelength where there is no significant absorption by meconium makes it possible to estimate the concentration of meconium. Observations have shown that light reflected from a sample of the fluid at 405 to 420nm increases with meconium concentration until a certain point (which is not necessarily the same from one sample to the next), where it starts to decrease due to the absorbing properties of meconium in that range. In contrast, reflectance values at, for example, 700nm continue to increase up to the maximum concentration measured (100g per litre of meconium). Blood can be differentiated in a similar way by measuring the reflectance at a third wavelength where blood absorbs light but meconium does not (540nm has been found to be suitable) and also at 700nm, where like meconium its

absorptance is small. Although Figure 1 may suggest at first sight that light absorptance by blood at 700nm is significant, the spectrum at 700nm is, in fact, the overall attenuation of a light beam due to both absorption and scattering of light. According to the Beer Lambert Law, the intensity I of a monochromatic light beam of initial intensity I_0 passing through a medium of path length d and concentration c is:-

$$I = I_0 e^{-ad}$$

where a is the attenuation coefficient which is plotted in Figures 1 and 2. The attenuation coefficient is, in fact, the sum of the absorption and scattering coefficients and is related to concentration of the substance under investigation in the following way:-

$$a = (a_1 + a_2)c$$

where a_1 is the absorption coefficient and a_2 is the scattering coefficient.

The scattering coefficient for blood is much larger than for meconium, but the absorption coefficients of both meconium and blood are insignificant at 700nm and can be ignored. Therefore, 700nm provides a suitable base line for concentration determinations when using reflectance measurements for both blood and meconium by logarithmic treatment of the reflectance measurements at 405 to 420nm, 540nm and 700 nm. Thus, by measuring the intensity of the illuminating light (and its spectral content), the

intensity of incident light at each wavelength of interest
(e.g. 405-420, 540 & 700nm) can be calculated. Using
these values and the values of reflected light at the same
three wavelengths, the reflection due to the vernix
content can be allowed for and compensated reflectance
values calculated which are related to the content of
meconium and blood in the amniotic fluid. From these
compensated values, the concentration of meconium and
blood can be calculated with a reasonable degree of
accuracy.

Optical measurements can be conveniently made in
vivo, using a flexible intrauterine probe of the kind
described in British patent application No. 8723605
(Publication No. 2195897). This is illustrated
diagrammatically in Figure 3. As described in our above
application, the probe is moulded from a suitable plastics
material such as polyurethane and is stiff and resilient
enough to enable it to be inserted by pushing into the
uterus from the proximate end through the cervix and
around the fetal head. The shape and dimensions and
mechanical properties of the body of the probe are
preferably as described in UK Patent Specification No.
2195897, the disclosure of which is incorporated herein.
Optical measurements are made using an optical cell which
is encapsulated in a potting composition from which the
probe is formed. The optical cell is preferably

constructed in such a way that fluid can flow from one side of the probe through to the other by passing through passages in the cell. Thus referring to Figure 3, the optical cell 31 is encapsulated in the body 32 of the probe and the cell is optically connected to an optic fibre bundle 33, also encapsulated in the body 32. Bundle 33 emerges from the proximate end of the probe from which it is optically connected (indicated diagrammatically in Figure 5) to photodetectors.

The cell is shown in Figure 4 and is manufactured in two inter-engaging parts (41 & 42). Figure 4 shows the cell in an exploded view. Part 42 includes a bore 43 (typically about 3mms in diameter), for receiving the fibre optic bundle 33 (not shown in Figure 4). The fibre optic bundle comprises a large number of optic fibres which are located in bore 43 and preferably sealed in place with a suitable thermoplastic resin, e.g. an epoxy resin to prevent ingress of amniotic fluid by capillary action. Suitable optic fibre bundles are supplied by Fibre Data Limited, Unit 8, Pool Industrial Estate, Druids Road, Redruth, Cornwall TR15 3RH. The particular fibre bundle employed contained about 540 silica fibres and was randomly divided into two equal branches (known as a 'Y' shape bifurcated bundle), one branch serves to transmit light into the optical cell and the other collects the reflected light and conveys it to the spectrophotometer,

comprising the photodetectors.   When assembled, part 42
is secured to part 41 by the screws or studs indicated.
Part 41 is shaped to provide conical or triangular-shaped
counter-surfaces which prevent light which strikes such
surfaces from being reflected back into the optic fibre-
ends 45 of bore 43.   Preferably, the internal faces 44
are coated with an anti-reflecting material or are
roughened to minimise reflection.

When encapsulated in the material forming the body of
the probe, faces 46 & 47 of parts 41 & 42 will be parallel
with the flat surfaces 35 of the probe and flanges 48 &
48A of parts 41 & 42 will serve to lock the parts into the
body of the probe.   However, a passage 38 remains open
through the probe and cell so that in use amniotic fluid
may pass through the cell from one side of the probe to
the other.   Because the flat face 35 of the probe will in
use lie against the wall of the uterus, light cannot be
reflected from the uterus into the optic fibre bundle
which is important since the wall of the uterus is red and
would give a spurious signal.

Figure 5 shows a block diagram of the processing
system.   As illustrated in the block diagram, light from
the source is fed to the probe via the optic fibre bundle
and a first light detector is linked to the light source
and measures its intensity.   Reflected light is returned
from the probe to second, third and fourth photodetectors

(which may be photodiodes) and are tuned to detect the
reflectance values at the three wavelengths of interest,
i.e. 405-420nm, 540nm, and 700nm, respectively.   After
amplification, the signals are fed via an analogue
multiplexer and an analogue-digital converter to a
microcomputer.

The light source used to illuminate the sample
passing the optical cell may be any suitable light source
of sufficient intensity at the three desired wavelengths.

Preferably, the light source is a tungsten halogen
filament bulb, although any light source emitting light at
415, 540 and 700nm would be suitable.   The tungsten
halogen lamp has the advantage that, while the total
intensity fluctuates with temperature, the spectral
content remains constant.   Thus, by measuring overall
intensity, the intensity delivered at each of the three
selected wavelengths can easily be calculated.

The optical components and electronics circuitry can
be housed together in a box adjacent to the bed and linked
to probe.   The output from this box may be taken to a
central processing unit such as a microcomputer via a
suitable interface.   This arrangement enables the
compensated reflectances to be calculated automatically
and in real time, logged and displayed on a VDU or any
suitable display in terms of corresponding concentrations
of meconium and blood, or a hard copy record to be

13

produced.   Alternatively, a simpler read-out can be
employed which merely gives an indication, when meconium
and/or blood is detected at a level which suggests cause
for alarm.

CLAIMS

1. A non-invasive system for monitoring the content of amniotic fluid during labour which comprises an optical cell supported in a probe capable of insertion into the uterus during labour, said cell being connected optically to a source of light (having a suitable spectral bandwidth) and to photodetecting means for detecting the spectral response of the amniotic fluid to illumination with said source and processing means for determining the presence of meconium and/or blood in the amniotic fluid by analysis of the spectral response.

2. A system according to claim 1 in which the cell is orientated in the probe in such a way that the amniotic fluid is illuminated by said light source while avoiding any reflection of light from the wall of the uterus reaching the photodetecting means.

3. A system according to claim 1 or claim 2 in which the optical cell is connected to the photodetecting means and to the light source by fibre optic cable.

4. A system according to claim 3 in which the fibre optic cable comprises a bundle of intermingled fibres, some of said fibres being optically connected at the end remote from the cell with the light source and others with the photodetecting means.

5. A system according to any one of the preceding claims in which the spectral response is analysed by

determining the light reflected at first and second
wavelengths at which meconium and blood, respectively,
strongly absorb light and at a third wavelength at which
meconium and blood do not absorb light significantly.

6.   A system according to claim 5 in which the first
wavelength is about 405 to 420 nm, the second wavelength
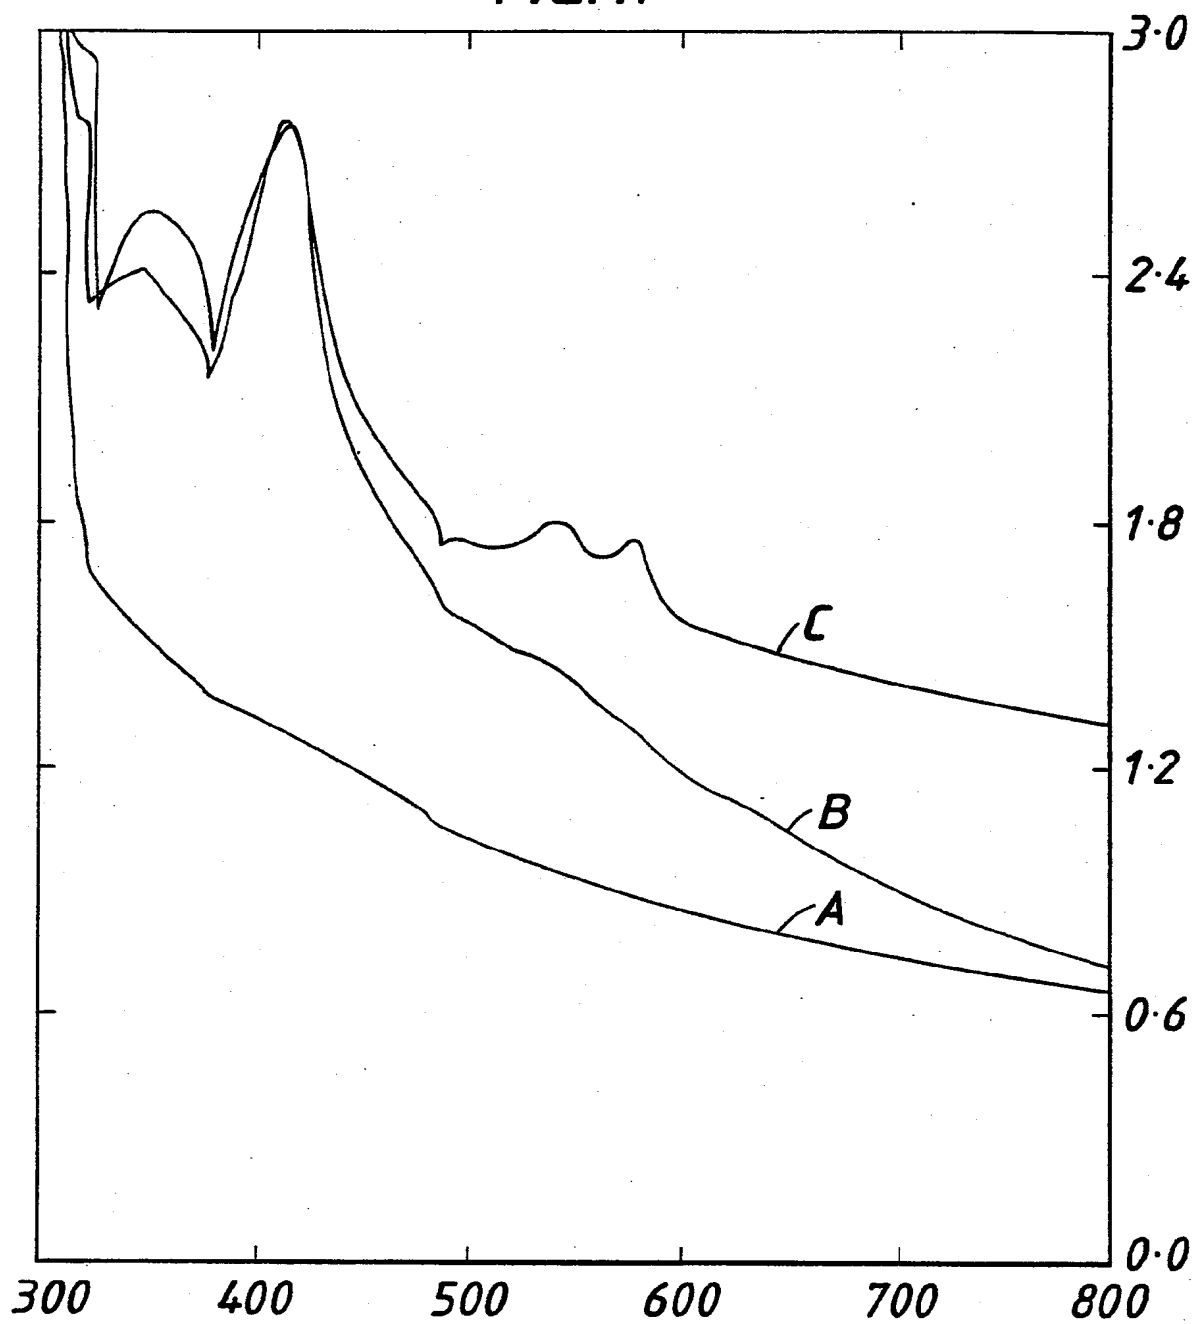is about 540 nm and the third wavelength is about 700 nm.

7.   An intrauterine probe which comprises a flexible
elongated body and an optical cell housed therein, the
cell being optically connected by fibre optic cable to the
distal end and the cell being located in the housing so
that in use amniotic fluid is able to pass through the
cell.

8.   A probe according to claim 7 wherein the
interior of the cell is provided with non-reflecting
surfaces.

9.   A probe according to claim 7 or 8 in which the
fibre optic cable comprises a bundle of fibres, some of
the fibres serving to transmit light and others to convey
light reflected by the amniotic fluid to the proximal end
for detection by photodetecting means, the fibres which
transmit light and the fibres which receive reflected
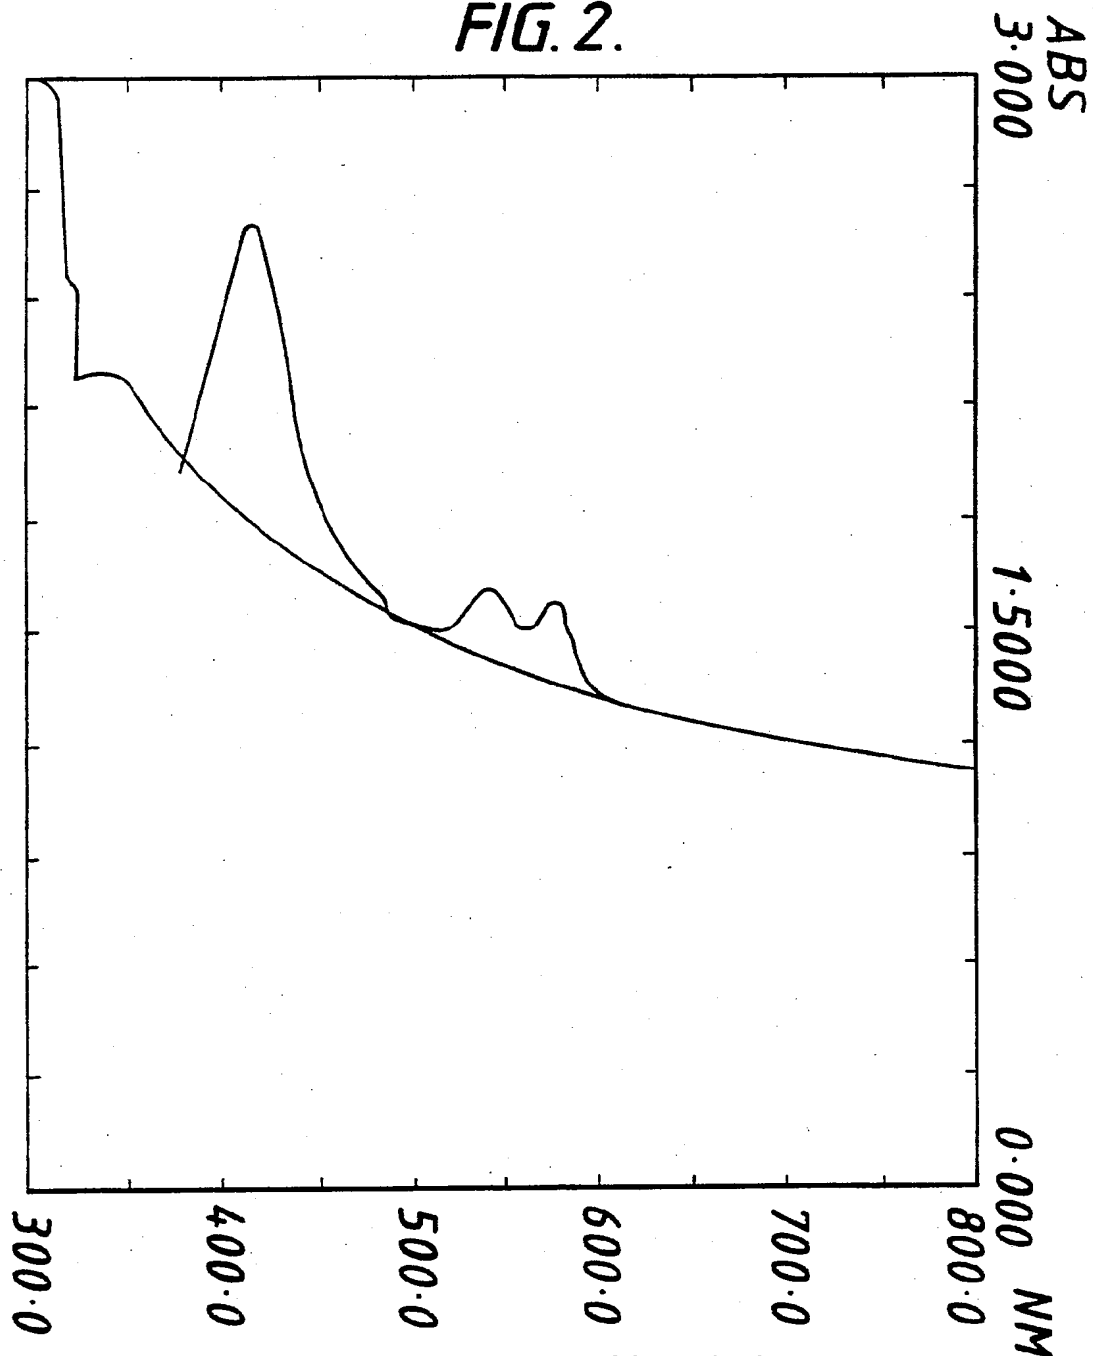light being intermingled in the bundle.

FIG.1.

2/4

FIG.2.

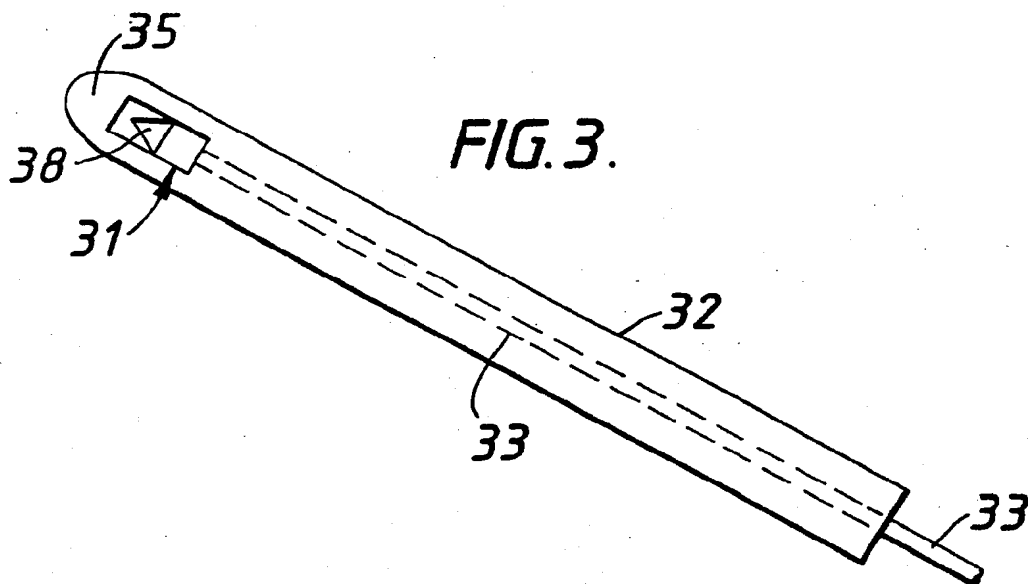Blood stained amniotic fluid
spectrum with expected baseline.

3/4
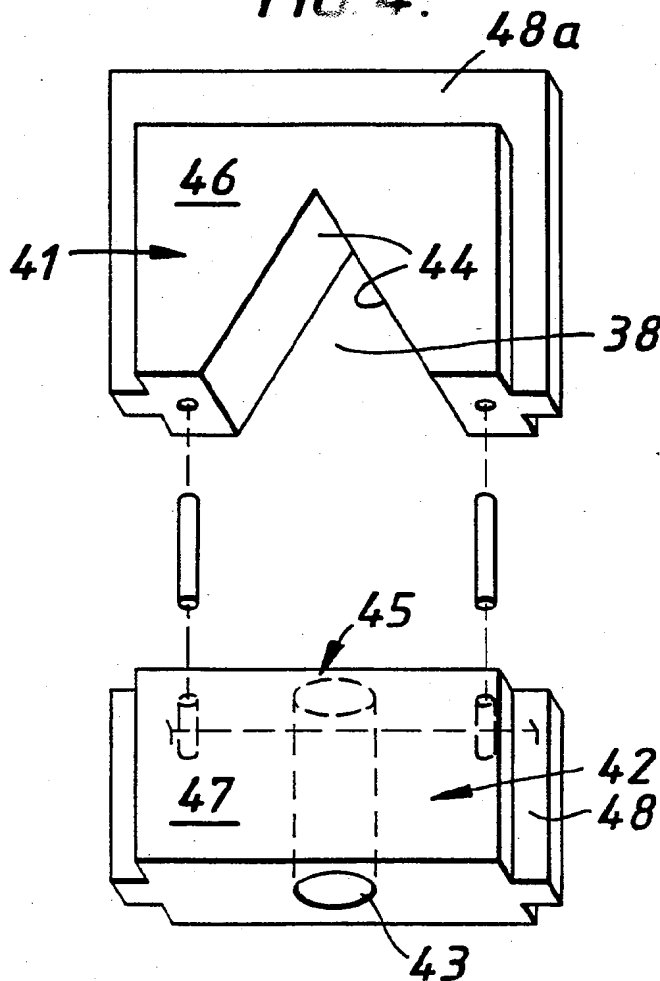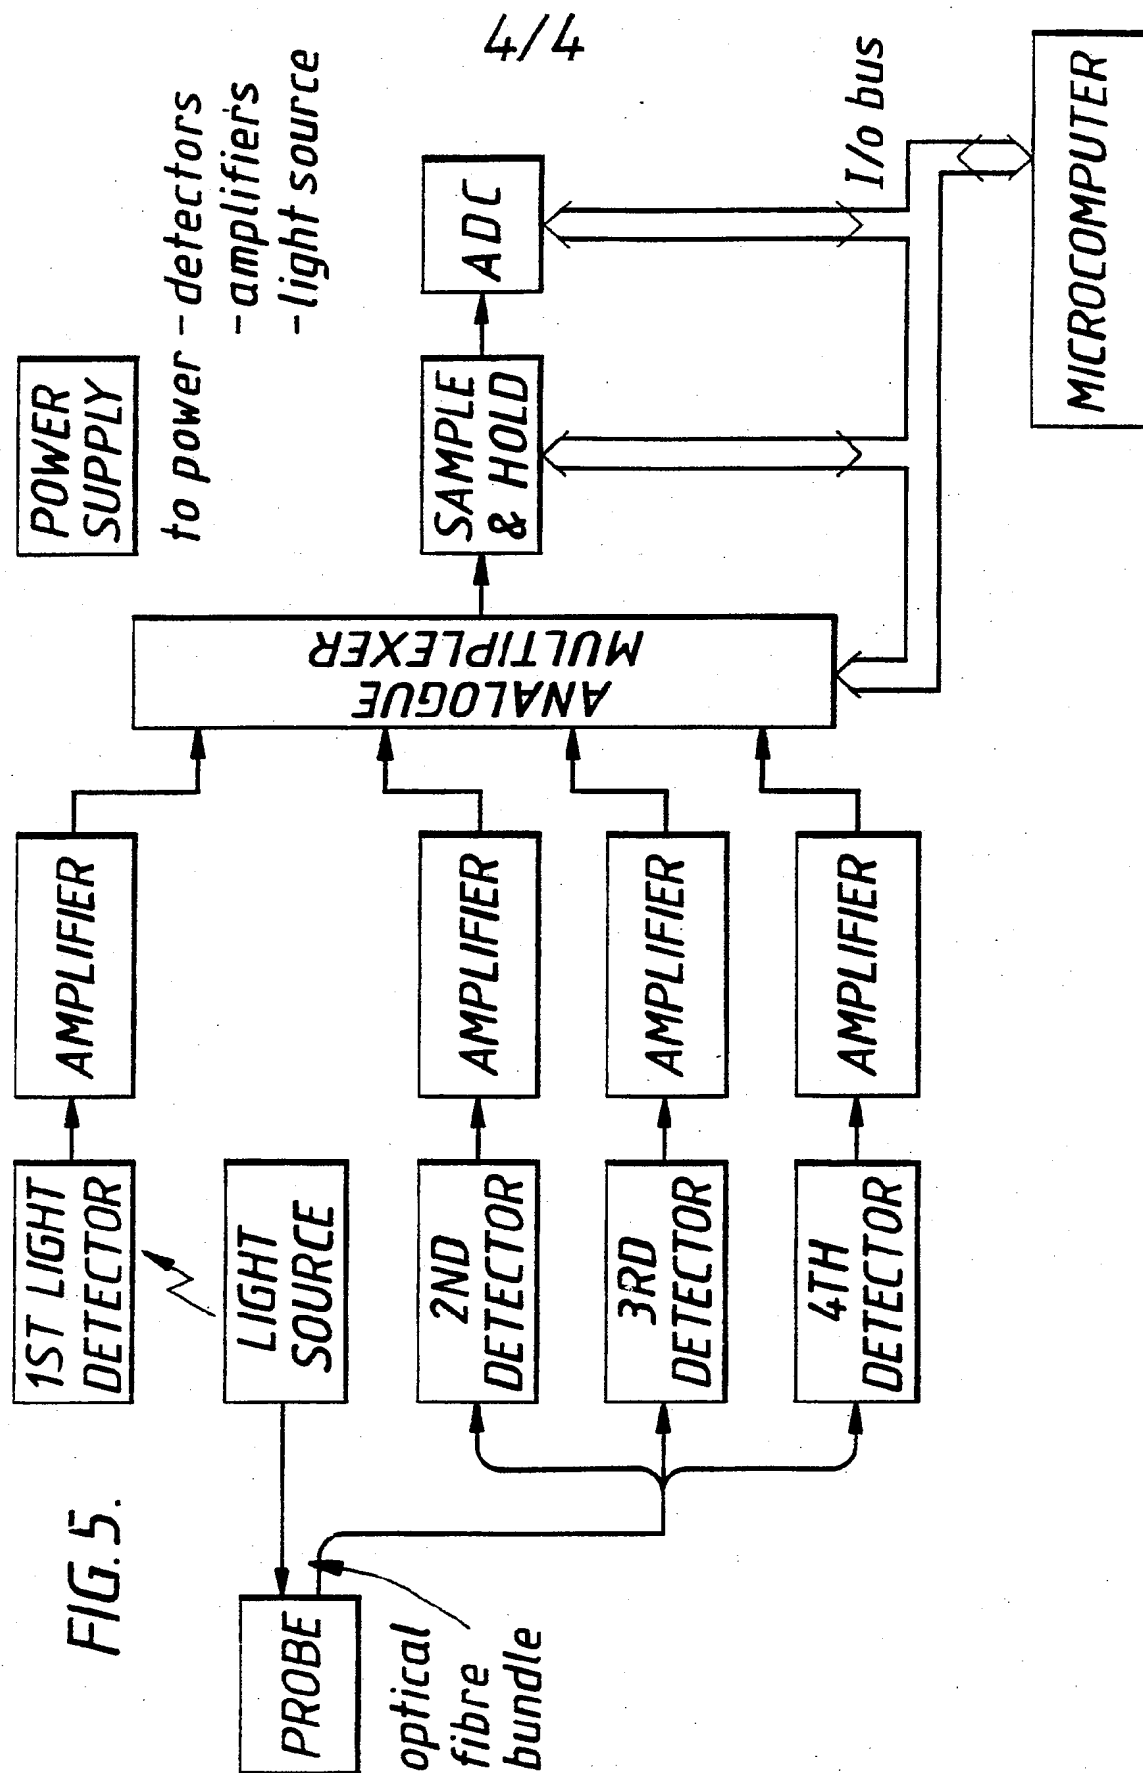
FIG.3.

FIG 4.

4/4

FIG.5.

I. CLASSIFICATION OF SUBJECT MATTER   (if several classification symbols apply, indicate all)[6]

According to International Patent Classification (IPC) or to both National Classification and IPC

Int.Cl. 5   A61B5/00

II. FIELDS SEARCHED

Minimum Documentation Searched[7]	
Classification System	Classification Symbols
Int.Cl. 5	A61B

Documentation Searched other than Minimum Documentation
to the Extent that such Documents are Included in the Fields Searched[8]

III. DOCUMENTS CONSIDERED TO BE RELEVANT[9]		
Category°	Citation of Document,[11] with indication, where appropriate, of the relevant passages[12]	Relevant to Claim No.[13]
X A	FR,A,2 608 909 (G.KARCHER ET AL.) July 1, 1988 see the whole document ---	1 2-9
A	GB,A,2 195 897 (ST. MARY'S HOSPITAL MEDICAL SCHOOL) April 20, 1988 cited in the application see the whole document ---	7-9
A	EP,A,063 431 (M.KONOMI) October 27, 1982 see the whole document ---	1-9

° Special categories of cited documents :[10]

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

IV. CERTIFICATION	
Date of the Actual Completion of the International Search	Date of Mailing of this International Search Report
09 OCTOBER 1991	1 9 NOV 1991
International Searching Authority	Signature of Authorized Officer
EUROPEAN PATENT OFFICE	HUNT B.W.

ANNEX TO THE INTERNATIONAL SEARCH REPORT
ON INTERNATIONAL PATENT APPLICATION NO.

GB   9101090
SA   49250

This annex lists the patent family members relating to the patent documents cited in the above-mentioned international search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

09/10/91

Patent document cited in search report	Publication date	Patent family member(s)		Publication date
FR-A-2608909	01-07-88	EP-A-	0276618	03-08-88
		US-A-	4856527	15-08-89
GB-A-2195897	20-04-88	EP-A-	0325605	02-08-89
		WO-A-	8802616	21-04-88
		US-A-	5025787	25-06-91
EP-A-063431	27-10-82	JP-A-	57168141	16-10-82
		JP-C-	1513886	24-08-89
		JP-A-	58005631	13-01-83
		JP-B-	63064736	13-12-88
		US-A-	4505583	19-03-85
		DE-A-	3277548	03-12-87